


5973 Air and Water Check

Instrument: MSD22  
 Fri Aug 04 08:27:34 2006

C:\MSDCHEM\1\5973N\

Scan: 10.00 - 75.00 Samples: 8 Thresh: 0 Step: 0.10  
 69 peaks Base: 69.00 Abundance: 339072

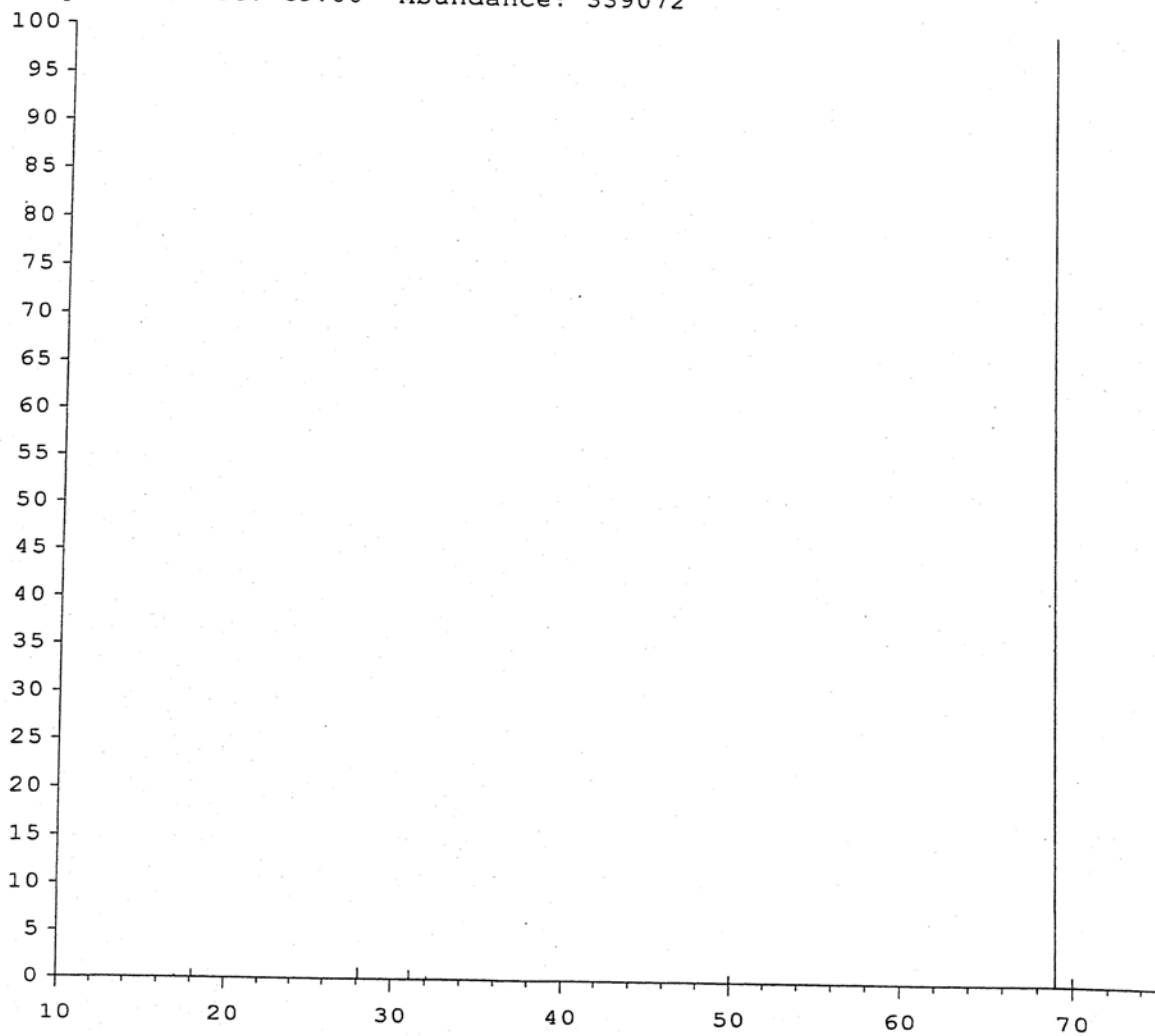

Mass	Abund	Rel Abund	Iso Mass	Iso Abund	Iso Ratio
69.00	339072	100.00	70.00	3659	1.08
18.10	2819	0.83	19.00	32	1.14
28.10	4239	1.25	29.00	101	2.38

Current Params used: ATUNE.U

Relative abundances:

18/69 = 0.83	Water%
28/69 = 1.25	Nitrogen%
32/69 = 0.43	Oxygen%
44/69 = 0.06	Carbon Dioxide%
28/18 = 150.37	Nitrogen/Water%